




Analysis of Odorant

Analysis Condition

Detector: FPD(filter:393nm)

Gas sampling valve (loop size=5ml) – Valve on time:0.5min

Column: SPB-1 sulfur(30m x 0.53mm x 4um)

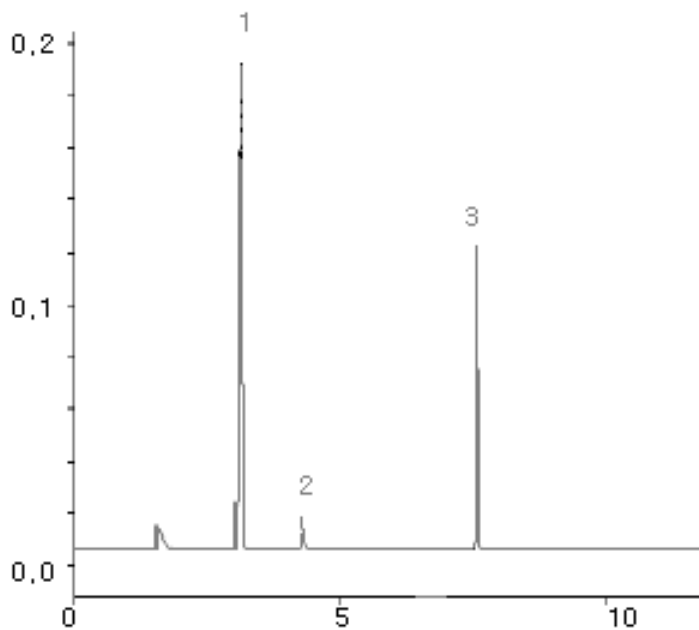

1. EM (Ethyl mercaptan) 9.8ppm

2. TBM (tert-butyl mercaptan) 3.2ppm

3. THT (tetrahydrothiophene) 6.8ppm