



## *Analysis of Pesticides in Potable Water*


### **Analysis Condition**

**Detector:** NPD

**Sample preparation:** liquid-liquid extraction

**Column:** HP-1(30m x 0.25mm x 0.25um)

**Oven temp.:** 150°C(1min) → 4°C/min → 250°C(10min)

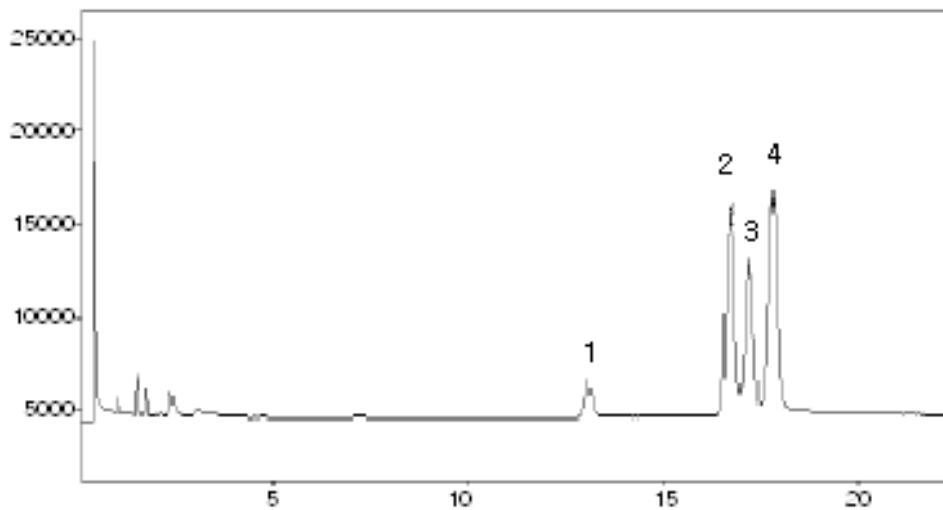

1. Diazinon
2. Fenitrothion
3. Malathion
4. Parathion